
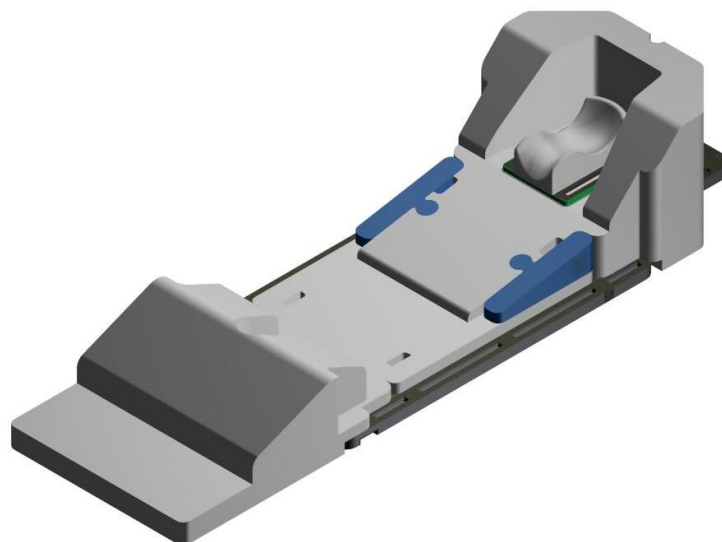


THE AIO SOLUTION® BREAST- & LUNGBOARD SOLUTION - THORAX ABDOMEN - LATERAL SUPPORTS

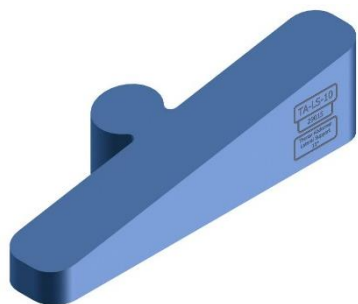

Article Nos. :

29012-V2 (R) & 29013-V2 (L) (AIO SOLUTION® code : **TA-LS-5**)

29014-V2 (R) & 29015-V2 (L) (AIO SOLUTION® code : **TA-LS-10**)

29016-V2 (R) & 29017-V2 (L) (AIO SOLUTION® code : **TA-LS-15**)

A. GENERAL PRODUCT INFORMATION

The products referred to in these instructions are medical devices used for patient positioning and immobilisation in radiation therapy.

To attain an optimal result, it is recommended to use these product in combination with Orfit immobilisation products.

B. PRODUCT DESCRIPTION

These BREAST- & LUNGBOARD – THORAX ABDOMEN LATERAL SUPPORTS (left and right) are a part of the “AIO SOLUTION BREAST- & LUNGBOARD PACKAGE”. They are used in combination with the other BREAST- & LUNGBOARD CUSHIONS, THE AIO SOLUTION BASE PLATES and EFFICAST PRE-CUTS to form a reproducible patient positioning and immobilisation system. Information on these other parts and instructions on how to make the masks can be found in the respective ‘instructions for use’ and on www.orfit.com.

C. PRECAUTIONS FOR USE

Always use these cushions in combination with the other AIO SOLUTION BREAST- & LUNGBOARD CUSHIONS on one of the base plates.

The cushions have positioning pieces on their sides that fit into the positioning holes of the THORAX ABDOMEN WEDGES (5° - 10° - 15° wedge). Always verify that the lateral supports are positioned correctly on the appropriate wedge. Do not expose these cushions to a hot air blower and make sure that no sharp objects can come into contact with these cushions.

It is not recommended to treat head and neck patients on the blue AIO cushions.

D. STORAGE

Always store the product in a safe place to prevent it from getting damaged. Do not put heavy objects on the cushion and prevent hard objects from falling onto it, because these will cause permanent deformations.

Store the cushions between +10°C (50°F) and 40°C (122°F).

E. PROPERTIES

E.1. Basic Physical Properties

The following physical properties apply to these cushions:

Density: Foam: 29 kg/m³
Coating: > 1 g/cm³

Dimensions: 5° : L 302 mm x W 80 mm x H 50 mm
10°: L 302 mm x W 80 mm x H 80 mm
15°: L 302 mm x W 80 mm x H 112 mm

Weight: 5°: 0,04 kg
10°: 0,06 kg
15°: 0,08 kg

E.2. Mechanical Properties

The AIO Cushions are made of low density PE foam that is covered with a PU coating. This combination results in a stable cushion that keeps its dimensions overtime and under conditions of frequent use.

The cushions used on the treatment machines are often used more frequently than those on the simulators and during the imaging stages. We therefore recommend rotating the sets between the different machines on a regular base to avoid differences in wear and tear of the cushions.

The maximum deformation measured after 100 uninterrupted pressure cycles with a compression strength of 500N on a surface of 5cm x 5cm is 28.1%. This corresponds to the force of 100 times per day the load of 50 kg applied with the palm of the hand.

E.3. Dosimetric Properties

The dosimetric build-up of this material (expressed in equivalent mmH₂O) depends largely on the length of the radiation pathway inside the cushion. Each mm of foam passed by the radiation beam will add 0.02 mmH₂O equiv. and each layer of coating that is passed will add another 0.35 mmH₂O equiv. to the total. The total can thus be calculated using the following formula:

$$\text{mmH}_2\text{O} = (L \times 0.02) + (n \times 0.35), \text{ where:}$$

L = length of the radiation pathway in the foam (in mm)

n = number of coating layers crossed by the radiation beam

The attenuation at 6MV and 15MV **per cm of material** through which the beam passes is:

Attenuation (± 0.15 %)	
6 MV	15 MV
0.12 %	0.09 %

Note: Use these numbers as a guidance only. Perform the measurements again in your department to verify these results.

F. MAINTENANCE AND WASTE MANAGEMENT


These products can be cleaned and disinfected by means of an isopropanol based disinfectant, applied with a soft cloth. If unsure about the cleaning fluid, do not use. **Never use aerosol sprays, corrosive cleaning agents, solvents or abrasive detergents. Do not soak the cushions.** Further cleaning instructions can be found in the [Orfit Cleaning Guidelines](#). Periodic checks of the product should be done to insure the parts are not worn and require repair or replacement. **Do not attempt to make repairs yourself.** Contact your distributor if there are any questions or concerns.

The products can be disposed of with household waste.


G. ADDITIONAL INFORMATION

The pictures (frontal view) below give an idea of the dimensions (height) of the complete Thorax and abdomen set and the minimum bore dimension (CT scanner etc.) needed for a clear pass into these tunnels. If a certain cushion setup cannot enter the tunnel, it is recommended to remove the armrest, slide the table through the tunnel and replace the armrest from the backside of the scanner.

The first view presents the highest setup possible (base plate, 0° cushion, 15° wedge and high armrest) together with two grip poles and the protruding handgrip:

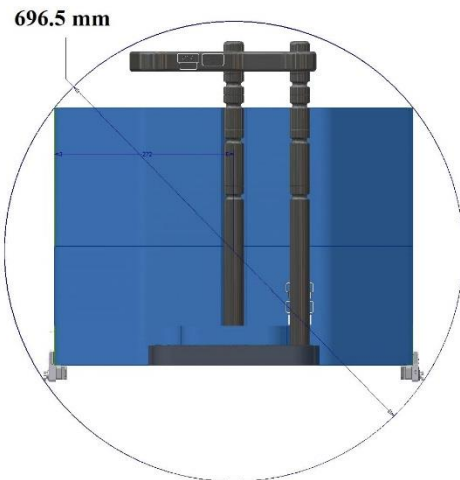

The second view is of a lower setup (base plate, 0° cushion, 5° wedge and high armrest):

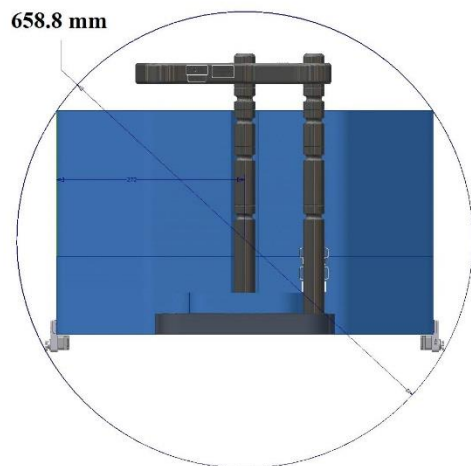

For additional information such as distributor contact information, product brochures, Safety Data Sheets and regulatory information, please visit our website www.orfit.com.

Note:

It is prohibited to make alterations to this text without prior approval from Orfit Industries. THE AIO SOLUTION® and EFFICAST® are registered trademarks of ORFIT INDUSTRIES N.V.



ORFIT INDUSTRIES
 Vosveld 9A | B-2110 Wijnegem | Belgium
 T (+32) (0)3 326 20 26
 welcome@orfit.com

www.orfit.com



Ref. No. 31921
 VERSION 7
 LAST UPDATE: 01/04/2021
 REVISION DATE: 01/04/2023